


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

JUN 07 2009


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130179
Name		John T. Ostoj	ID# 4823 Date 6/9/09
A	Agency	Alaska STATE TROOPERS	Phone # 262-4453
Instrument Location		Soldotna AST Post	
Alco S/N		X301540	Target Value .082 High Pressure 500
B	Alco Test Value Average	.083	.082
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature			
(OVER)			

BMB  
6/16/09


I, Nita J. Bolz, after being first duly sworn, depose and state as follows: (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.

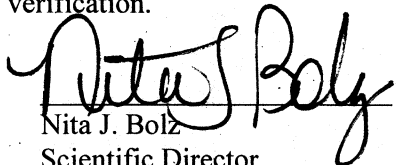


Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 24<sup>th</sup> day of June 2009.

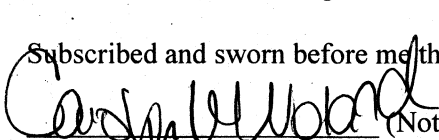  
(Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130179

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130179

JUNE 09, 2009

OPERATOR'S NAME:

OSTOJ/JOHN/T

OPERATOR'S NUMBER: 4823

SUBJECT'S LAST NAME:

TEST

SUBJECT'S FIRST NAME/MI :

UOC

O.L. #: TEST

DEPT/AGENCY: SLD0

CASE/REPORT: TEST

TEST TYPE: U

ALCO TARGET VALUE: .002

ALCO S/N: X301540

--- BREATH ANALYSIS ---

.002 ADJUSTED FOR 30.22 in

ALCO TARGET .002 07:38

BLANK TEST .000 07:39

INTERNAL STANDARD VERIFIED 07:39

ALCO TV 30.22 in .003 07:39

BLANK TEST .000 07:40

SUBJECT SAMPLE .000 07:41

BLANK TEST .000 07:41

ALCO TV 30.22 in .002 07:42

BLANK TEST .000 07:42

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130179

JUNE 09, 2009

TIME 07:34

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 30.22 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

11#021000-0107456789:0=>00000000  
HIJKLMN0PQRSTUWXYZ0123456789:0=>00000000  
pqrstuwxvzyz0123456789:0=>00000000